



中国认可
国际互认
检测
TESTING
CNAS L18131

Test Report

Report Number: 26060536-04-R01EN



Sponsor: Shenzhen Zhongchuang 3D Technology Co., Ltd

Factory: Dongguan Daji 3D Technology Co., Ltd.

Sample Name: Permanent crown resin

Model/ Specification: PRS-R-01

Test Category: Commission Test

EPINTEK Guiyang Ltd.

Declaration

1. The report is invalid without the special stamp for test report of the test facility.
2. Partial copy is invalid without written approval of the test facility.
3. Any copy is invalid without the special stamp of the test facility for test report.
4. The report is invalid without the signature of the authorized signatory.
5. The report is invalid once altered.
6. Any comment to the report should be submitted in writing to the test facility, otherwise it may not be accepted.
7. The results in this report are relevant only to the articles tested.
8. The sponsor is responsible for the authenticity of the sample and its information.

Facility Name: EPINTEK Guiyang Ltd.

Facility 1: Industrial Incubation Park, Dayang Road, Baiyun District, Guiyang, Guizhou, China

Telephone: 0851-84614538

Postal Code: 550014

Facility 2: No. 1, 4/F, Building 16.18, No.7888, Tongcheng Avenue, Baiyun District, Guiyang, Guizhou,

China

Telephone: 0851-84614538

Postal Code: 550016

Web site: www.epintek.com

EPINTEK Guiyang Ltd.

TEST REPORT

Report Number: 26060536-04-R01EN

Sample Name	Permanent crown resin	Sample ID	26060536
Model/ Specification	PRS-R-01		
Sponsor	Shenzhen Zhongchuang 3D Technology Co., Ltd		
Address	Room 204, Administration Building, Jia Tai Pharmaceutical, No.1 Industrial Zone,Tangwei Community, Fuhai Street, Bao'an District, Shenzhen City		
Factory	Dongguan Daji 3D Technology Co., Ltd./Room 401, Building 2, No. 6 Xiyi Street, Xingfa South Road, Wusha, Chang'an Town, Dongguan City		
Test Facility	EPINTEK Guiyang Ltd., Facility 1		
Test Category	Commission Test	Lot#	/
Produced Date	2026.06.06	Sample Quantity	14 PCS
Received Date	2026-06-17	Test Date(s)	2026-06-22~2026-06-26
Test Item(s)	<i>In Vitro</i> Cytotoxicity Test		
Test Method(s)	ISO 10993-5:2009 Biological evaluation of medical devices—Part 5: Tests for <i>in vitro</i> cytotoxicity		
Conclusion	Under the conditions of this study, the test sample extract did not show a potential cytotoxicity to L-929 cells. (Stamp for Test Report) Issued Date:		
Notes	"NA" means "not applicable","/"means "blank"		

Drafted by: _____
Sean Shao

Reviewed by: _____
Pearl Tu

Approved by: _____
Aspenn Zeng

Position: Authorized Signatory

EPINTEK Guiyang Ltd.

TEST REPORT

Report Number: 26060536-04-R01EN

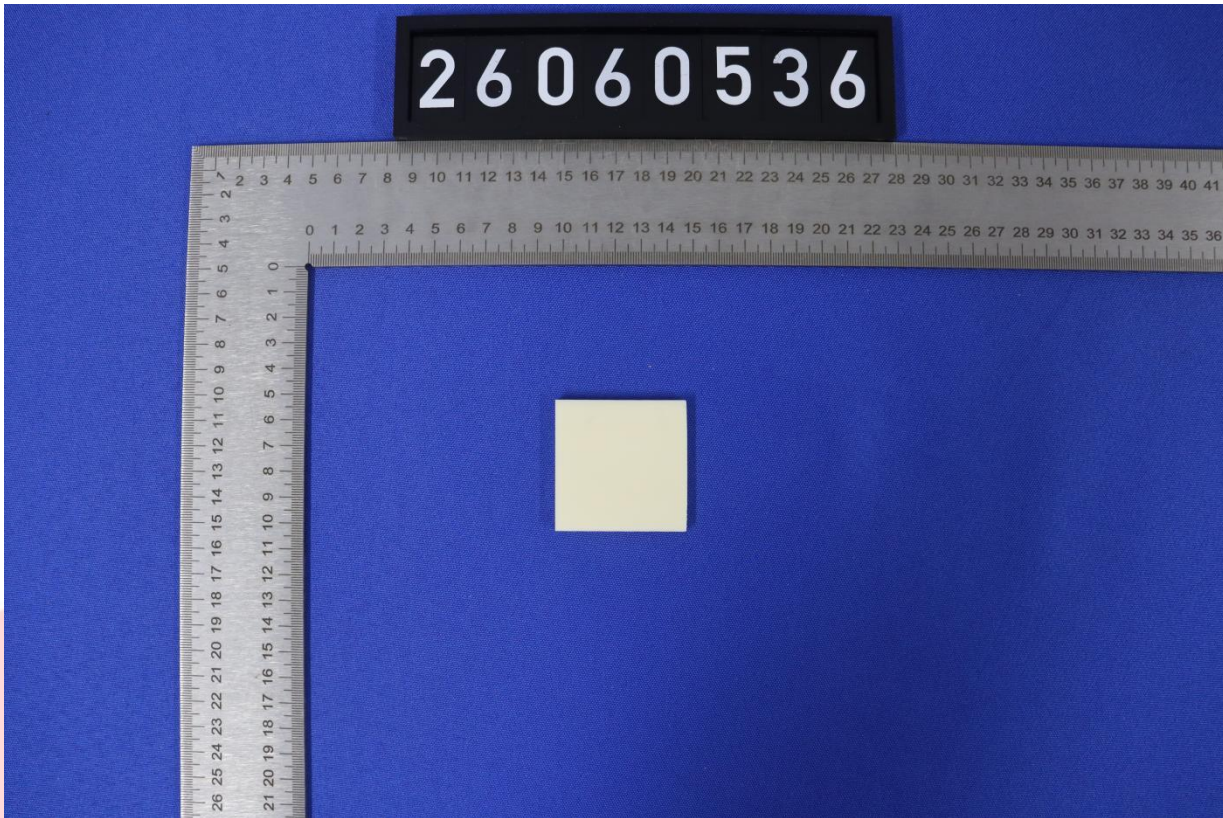
No.	Item	Standard Method	Acceptance Criteria	Test Result	Conclusion	Note
1	<i>In Vitro</i> Cytotoxicity Test	ISO 10993-5:2009 MTT Method	If cell viability less than 70 %, the sample extract has a cytotoxic potential.	Under the conditions of this study, the 100% extracts of the test sample viability was 81.7%.	Under the conditions of this study, the test sample extract did not show a potential cytotoxicity to L-929 cells.	Details Shown in Annex

EPINTEK

EPINTEK Guiyang Ltd.

TEST REPORT

Report Number: 26060536-04-R01EN

Picture of Sample

Description for Sample, Model/Specification
Initial State: Unsterilized Physical State: Solid (Note: The above information was provided by the sponsor)
Misc
None

Annex of Test Report

***In Vitro* Cytotoxicity Test- MTT Method**

Study No.: 26060536-003506

Model/ Specification: PRS-R-01

Lot#: /

EPINTEK Guiyang Ltd.



SUMMARY

1. Purpose

The purpose of the test is to determine cytotoxic potential of the test sample extract on L-929 cells.

2. Test Procedure

The test sample (Overall sampling) is extracted in complete MEM medium supplemented with 10% fetal bovine serum (FBS) at an extraction ratio of 3 cm²/ mL for 72 hours in a constant temperature shaking incubator at 37 °C. The negative control and positive control are extracted under identical incubation conditions at ratios of 3 cm²/mL and 6 cm²/mL respectively. The medium control is extracted alongside the test sample under the same conditions.

On Day 1, L-929 cell suspension is seeded into 96-well plates and incubated in an incubator (5% CO₂, 37 °C, relative humidity >90%) for 24 hours. On Day 2, the culture medium is aspirated, and serially diluted test sample extracts (100%, 75%, 50%, 25%) are added to each well separately. The plates are incubated for another 24 hours at 37 °C with 5% CO₂.

After the 24- hour incubation period, cell morphological observation is carried out first. Subsequently, 50 µL of MTT solution (1 mg/mL) is added to each well, followed by a 2- hour incubation, after which absorbance values are measured..

3. Test Result

The MTT test results showed that the cell viability of the 100% test sample extract was 81.7%. The results of control groups showed the test was valid.

4. Conclusion

Under the conditions of this study, the test sample extract did not show a potential cytotoxicity to L-929 cells.

1. Study Summaries

1.1. Purpose

The purpose of the test is to determine cytotoxic potential of the test sample extract on L-929 cells.

1.2. Deviation(s) and Incident(s) Procedure

If any deviation or incident has occurred in the test, the information will be recorded in a deviation report timely, and incorporated in this test report to evaluate the impact to final result(s).

1.3. Major Laboratory Personnel

Study Director: Eartha Zhang

Engineers: Sean Shao

1.4. Study Dates

Test Start: 2026-06-22

Test End: 2026-06-26

Report Completed: 2026-07-09

2. Testing Information

2.1. Blank Control

Name: MEM with 10% FBS

Manufacturer: ExCell (FBS); HyClone (MEM)

Lot/ Batch#: 012E-0515A (FBS); AL30859021 (MEM)

Size: 500 mL (FBS); 500 mL (MEM)

Physical State: Liquid

Color: Red

Storage Condition: (2~8) °C

Extracting Condition: 37 °C, 72 h, 60 rpm

2.2. Negative Control

Name: High Density Polyethylene Film
Manufacturer: Hatano Research Institute, FDSC
Lot/ Batch#: C-212
Size: c.a.3 cm ×10 cm (5 sheets)
Physical State: Solid
Color: White
Storage Condition: Room temperature
Extracting Ratio: 3 cm²/1 mL
Extracting Condition: 37 °C, 72 h, 60 rpm

2.3. Positive Control

Name: No powder latex gloves
Manufacturer: GFM World Sdn.Bhd.
Lot/ Batch#: 202411DWL656
Size: S
Physical State: Solid
Color: White
Storage Condition: Room temperature
Extracting Ratio: 6 cm²/1 mL
Extracting Condition: 37 °C, 72 h, 60 rpm

2.4. Instruments and Reagents

2.4.1. Main Instruments

Name	No.	Calibration Due Date
CO ₂ Incubator	EPME-068	2027-04-08
Clean Bench	EPME-108	2027-03-30
Constant Temperature Shaking Incubator	EPME-061	2027-02-27
Micro-plate Reader	EPME-063	2027-05-13
Inverted Microscope	EPME-051	Check qualified

2.4.2. Main Reagents

Name	Lot#	Manufacturer
Fetal bovine serum (FBS)	012E-0515A	ExCell
Minimum essential medium (MEM)	AL30859021	HyClone
Penicillin, Streptomycin	20250911	NCM Biotech
Trypsin	2503821	BLOEXPLORER
3-(4,5-Dimethyl-2-Thiazolyl)-2,5-Diphenyl Tetrazolium Bromide (MTT)	C18575851	MACKLIN
MEM (without phenol red)	251130	GenXion
Isopropanol	20251129	Fuyu

3. Justification of the Test System

L-929 cells have been used for cytotoxicity because they demonstrate sensitivity to extractable cytotoxic samples.

4. Identification of the Test System

L-929 cells obtained from Procell Life Science& Technology Co.,Ltd.

5. Route of Exposure

Exposing the test sample to the test system via its extract (extracted using a carrier compatible with the test system) is regarded as the optimal contact route and is recommended by the standard.

6. Test Design

6.1. Preparation of Extracts

Table 1 Extraction Condition

Aseptically Sampling			Media	Sterilization Method	Extract Condition ²⁾
Ratio	Sampling Method ¹⁾	Sample Amount			
3 cm ² / mL	Overall sampling	50 cm ²	MEM with 10% FBS	Alcohol disinfection (Soak)	37 °C, 72 h, 60 rpm

Table 2 Extraction Details ³⁾

Volume	pH	Clear	Color Change	Particle or precipitate	Centrifugation, Filtration or pH adjustment
16.66 mL	7.34	Clear	Not	Not	Not

- 1) Surface area of a single sample: 50 cm² (Provided by the sponsor), One sample was used in this test.
- 2) The extraction process was conducted in a shaking machine.
- 3) The result extracts were used immediately.

6.2. Preparation of MTT solution

MTT is dissolved in MEM without supplements and without phenol red at a concentration of 1 mg/mL. This solution is sterilized by filtering with 0.22 µm membrane, the solution should be used the same day.

6.3. Test Procedure

L-929 cells were cultured in MEM medium (10% FBS, Penicillin 100 IU/mL, Streptomycin 100 µg/mL) in cell incubator (5% CO₂, 37°C, >90% humidity), then digested with 0.25% trypsin to get single cell suspension. And obtained a 1×10⁵ cells/mL suspension by centrifuging (200 g, 3 min) and re-suspended in MEM medium finally. The suspended cells were dispensed at 100 µL per well in 96-well plate, and cultured it in cell incubator (5% CO₂, 37°C, >90 % humidity) for 24h, cell morphology was evaluated to verify that the monolayer was satisfactory.

After the cells grew to form a monolayer, original culture medium was discarded. The 96-well plates were then treated with 100 µL extract of test sample (100%, 75%, 50%, 25%), blank control, negative control (100%) and positive control (100%) respectively. Incubated the 96-well plate in cell incubator (37°C, 5% CO₂, >90 % humidity) for another 24 h. Six parallel wells of each test were tested.

After 24 h incubation, take out the 96-well plate for cell morphology observation first, and then discard the original culture medium. 50µL aliquot of MTT (1 mg/mL) was added to each well and then incubated in cell incubator (37°C, 5% CO₂, >90% humidity) for 2 h. The supernatant in each well was tipped out and 100 µL isopropanol was added to each well.

Evaluated the absorbance value with a micro-plate reader with the measurement wavelength at 570nm and reference wavelength at 650nm.

7. Data analysis and calculation

Mean±standard deviation ($\bar{X} \pm SD$)

$$\text{Viab.}\% = \frac{100 \times OD_{570e}}{OD_{570b}}$$

OD_{570e} —is the mean value of the measured optical density of the extracts of the test sample;

OD_{570b} —is the mean value of the measured optical density of the blanks.

8. Evaluation Criterion

- The lower the Viab.% value, the higher the cytotoxic potential of the test item is.
- If viability is reduced to 70 % of the blank, the test sample extract has a cytotoxic potential.
- The 50 % extract of the test sample should have at least the same or a higher viability than the 100 % extract; otherwise the test should be repeated.

9. Alteration and Deviation

No deviation affecting the validity of the test data occurred.

10. Results

10.1. Results of Cell Morphology

Table 3 Observation of cell morphology

Group	Before treated with extract	24 h after treatment
Blank control		Discrete intracytoplasmic granules, no cell lysis, no reduction of cell growth.
Negative control		Discrete intracytoplasmic granules, no cell lysis, no reduction of cell growth.
Positive control		Nearly complete or complete destruction of the cell layers.
100% Test sample extract	Discrete intracytoplasmic granules, no cell lysis, no reduction of cell growth.	Not more than 20 % of the cells are round, loosely attached and without intracytoplasmic granules, or show changes in morphology; occasional lysed cells are present; only slight growth inhibition observable.
75% Test sample extract		Not more than 20 % of the cells are round, loosely attached and without intracytoplasmic granules, or show changes in morphology; occasional lysed cells are present; only slight growth inhibition observable.
50% Test sample extract		Not more than 20 % of the cells are round, loosely attached and without intracytoplasmic granules, or show changes in morphology; occasional lysed cells are present; only slight growth inhibition observable.
25% Test sample extract		Discrete intracytoplasmic granules, no cell lysis, no reduction of cell growth.

10.2. Results of Cell Vitality

Table 4 Results of cell viability

Group	$\bar{X} \pm SD$	Viability
Blank control	0.682±0.016	100.0%
Negative control	0.668±0.005	97.9%
Positive control	0.023±0.008	3.4%
100% test sample extract	0.557±0.007	81.7%
75% test sample extract	0.579±0.023	84.9%
50% test sample extract	0.595±0.026	87.2%
25% test sample extract	0.618±0.022	90.6%

11. Conclusion

Under the conditions of this study, the test sample extract did not show a potential cytotoxicity to L-929 cells.

12. Archiving

All related documents, study protocol, test report and raw data, including the documentation, printouts of instruments and computers, are stored in the archiving room of the test facility.

.....End of the Report.....